


Valved Entry System



Valved cannula provides a closed system, eliminating the need for plugs and decreasing instrument exchanges

- EDGEPLUS[®] blade delivers a flat linear incision
- Cannula removes easily from trocar after insertion without secondary instrument
- Low friction silicone valves designed for smooth instrument exchange
- Locking mechanism on trocar hub provides for rotational control of cannula during insertion

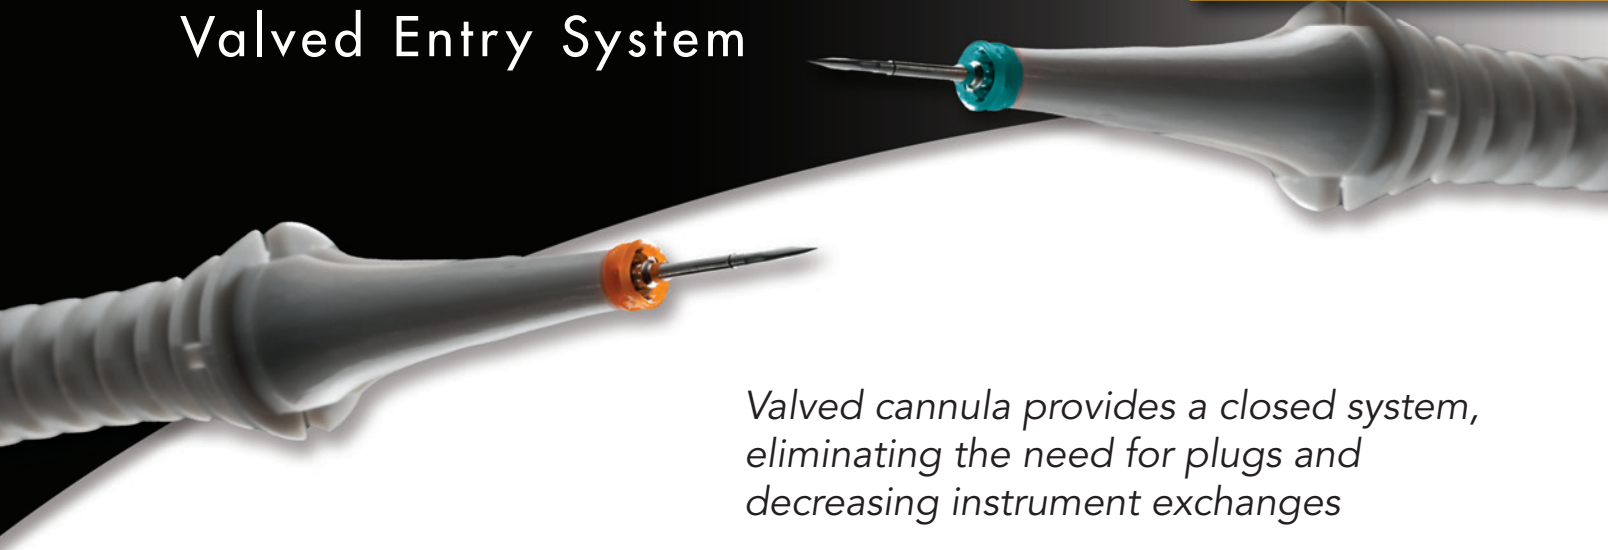

Vent is provided with each set for cases requiring silicone oil or perfluorocarbon liquids.



23G VALVED ENTRY SYSTEM

12/box


- | | |
|------------|-------------|
| 8065751585 | 1-Count 4mm |
| 8065751657 | 3-Count 4mm |
| 8065751800 | 1-Count 6mm |
| 8065751801 | 3-Count 6mm |



25G VALVED ENTRY SYSTEM

12/box

- | | |
|------------|-------------|
| 8065751586 | 1-Count 4mm |
| 8065751658 | 3-Count 4mm |
| 8065751782 | 1-Count 6mm |
| 8065751778 | 3-Count 6mm |

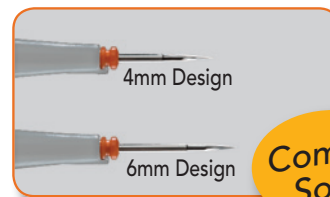

Coming Soon

Contact your local representative at 1-800-TO-ALCON (1-800-862-5266)
alconretina.com



CONSTELLATION[®] Vitreotomy Valved Cannula TOTAL PLUS[®] Pak

- Straight Endoilluminator
- Includes EDGEPLUS[®] Valved Entry System

NEW

8065751900 | 23G | 5000 CPM | 6/box
8065751902 | 25+™ | 5000 CPM | 6/box

23 25+

CONSTELLATION[®] Valved Cannula Combined Procedure Pak

- Straight Endoilluminator
- Tipless
- Includes EDGEPLUS[®] Valved Entry System

NEW

8065751908 | 23G | 5000 CPM | 0.9 mm | 6/box
8065751910 | 25+™ | 5000 CPM | 0.9 mm | 6/box

23 25+

CONSTELLATION[®] System 23G Stand Alone Components

23

CONSTELLATION [®] ULTRAVIT [®] 23 Gauge Vitrectomy Probe		
8065750949	6/box	5000 CPM
8065751585	12/box	EDGEPLUS [®] Valved Entry System (1 Ct)
8065751657	12/box	EDGEPLUS [®] Valved Entry System (3 Ct)
8065751800	12/box	6 mm EDGEPLUS [®] Valved Entry System (1 Ct)
8065751801	12/box	6 mm EDGEPLUS [®] Valved Entry System (3 Ct)
8065751446	12/box	EDGEPLUS [®] Trocar/Cannula Set (1 Ct)
8065751447	12/box	EDGEPLUS [®] Trocar/Cannula Set (3 Ct)
8065751444	12/box	6 mm EDGEPLUS [®] Trocar/Cannula Set (1 Ct)
8065751445	12/box	6 mm EDGEPLUS [®] Trocar/Cannula Set (3 Ct)
8065750842	6/box	Small Parts Kit (includes plugs, infusion cannula & adaptors)
8065750841	12/box	Infusion Cannula
8065750837	6/box	Plug Sets (3 Ct)

CONSTELLATION[®] System 25+™ Series Stand Alone Components

25+

CONSTELLATION [®] ULTRAVIT [®] 25+™ Vitrectomy Probe		
8065751438	6/box	5000 CPM
8065751586	12/box	EDGEPLUS [®] Valved Entry System (1 Ct)
8065751658	12/box	EDGEPLUS [®] Valved Entry System (3 Ct)
8065751782	12/box	6 mm EDGEPLUS [®] Valved Entry System (1 Ct)
8065751778	12/box	6 mm EDGEPLUS [®] Valved Entry System (3 Ct)
8065751448	12/box	EDGEPLUS [®] Trocar/Cannula Set (1 Ct)
8065751449	12/box	EDGEPLUS [®] Trocar/Cannula Set (3 Ct)
8065751780	12/box	6 mm EDGEPLUS [®] Trocar/Cannula Set (1 Ct)
8065751781	12/box	6 mm EDGEPLUS [®] Trocar/Cannula Set (3 Ct)
8065751442	6/box	Small Parts Kit (includes plugs, infusion cannula & adaptors)
8065751459	12/box	Infusion Cannula
8065751443	6/box	Plug Sets (3 Ct)

Indications for Use: The CONSTELLATION[®] Vision System is an ophthalmic microsurgical system that is indicated for both anterior segment (i.e., phacoemulsification and removal of cataracts) and posterior segment (i.e., vitreoretinal) ophthalmic surgery.

Caution: Federal (USA) law restricts this device to sale by, or on the order of, a physician.

Warnings and Precautions:

- Attach only Alcon supplied products to console and cassette luer fittings. Improper usage or assembly could result in a potentially hazardous condition for the patient. Mismatch of surgical components and use of settings not specifically adjusted for a particular combination of surgical components may affect system performance and create a patient hazard. Do not connect surgical components to the patient's intravenous connections.
- Each surgical equipment/component combination may require specific surgical setting adjustments. Ensure that appropriate system settings are used with each product combination. Prior to initial use, contact your Alcon sales representative for in-service information.
- Care should be taken when inserting sharp instruments through the valve of the Valved Trocar Cannula. Cutting instrument such as vitreous cutters should not be actuated during insertion or removal to avoid cutting the valve membrane. Use the Valved Cannula Vent to vent fluids or gases as needed during injection of viscous oils or heavy liquids.
- Visually confirm that adequate air and liquid infusion flow occurs prior to attachment of infusion cannula to the eye.
- Ensure proper placement of trocar cannulas to prevent sub-retinal infusion.
- Leaking sclerotomies may lead to post operative hypotony.
- Vitreous traction has been known to create retinal tears and retinal detachments.
- Minimize light intensity and duration of exposure to the retina to reduce the risk of retinal photic injury.

ATTENTION: Reference the Directions for Use labeling for a complete listing of indications, warnings, precautions, complications and adverse events.